




# The biomaterials people


## Glaucoma Valve

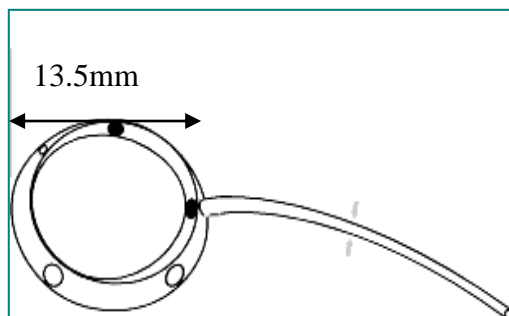

### SINGLE PLATE GLAUCOMA VALVE

**Material:** Silicone  
**Indications:** refractory glaucoma, failure of previous filtering surgery


**Product reference:**  
**S4-2000** Box of 1 (sterile)  
Supplied with calibrated needle and control cannula.

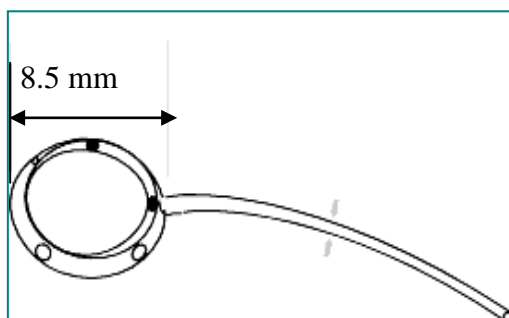

### PAEDIATRIC GLAUCOMA VALVE

**Material:** Silicone  
**Indications:** refractory glaucoma, failure of previous filtering surgery


**Product reference:**  
**S4-2050** Box of 1 (sterile)  
Supplied with calibrated needle and control cannula.

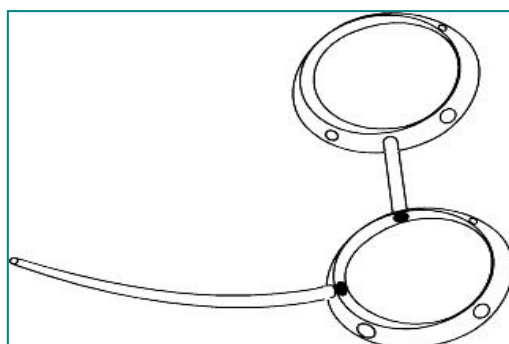

### RIGHT EYE DOUBLE PLATE GLAUCOMA VALVE

**Material:** Silicone  
**Indications:** refractory glaucoma, failure of previous filtering surgery

**Product reference:**  
**S4-2100** Box of 1 (sterile)  
Supplied with calibrated needle and control cannula.

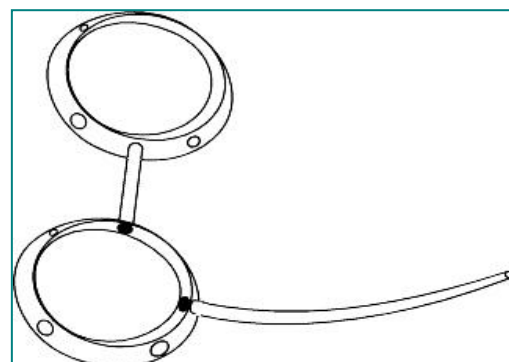

### LEFT EYE DOUBLE PLATE GLAUCOMA VALVE

**Material:** Silicone  
**Indications:** refractory glaucoma, failure of previous filtering surgery

**Product reference:**  
**S4-2200** Box of 1 (sterile)  
Supplied with calibrated needle and control cannula.



20/22, Rue Louis Armand  
75015 PARIS - France

Tél.: 33 (0) 1 53 98 98 97 E-mail [fciepx@fci.fr](mailto:fciepx@fci.fr)  
Fax: 33 (0) 1 53 98 98 99 Web: <http://www.fci.fr>